

**(PLEASE SWITCH TO THE SLIDE SHOW MODE)**

**Dräger X-am 5000 / X-am 5600**  
**VIDEO BASIC TRAINING**

Dräger, Lübeck 24.09.2009

# CONTENT


	<b>Page</b>		<b>Page</b>
 Disclaimer	4	 Menu – STEL	14
 Dräger X-am 5x00 Overview	5	 Recognising Different Alarms	15-23
 Switching On & Warming-Up Period	7	 Notice and Error Icons	24
 Switching Off	8	 Confined Space Entry	27
 Display Illumination	9	 Bump Test Station	32
 Menu – Fresh Air Calibration	10	 Manual Bump Test	33
 Menu – Maximum Value	11	 Charging Battery	34
 Menu – TWA	12	 Replacing Alkaline Battery	35
		 Overview of Icons	36

## General Information

**This visual presentation is intended to help the user understand and correctly use the Dräger X-am 5000/5600. It is not intended to be a substitute for the complete instruction manual supplied with the instrument.**

**IT IS THE USER'S RESPONSIBILITY TO READ AND UNDERSTAND ALL MANUALS AND INFORMATION PROVIDED WITH THE INSTRUMENTS!**

## Dräger X-am 5000/5600 Basic – Components on Front

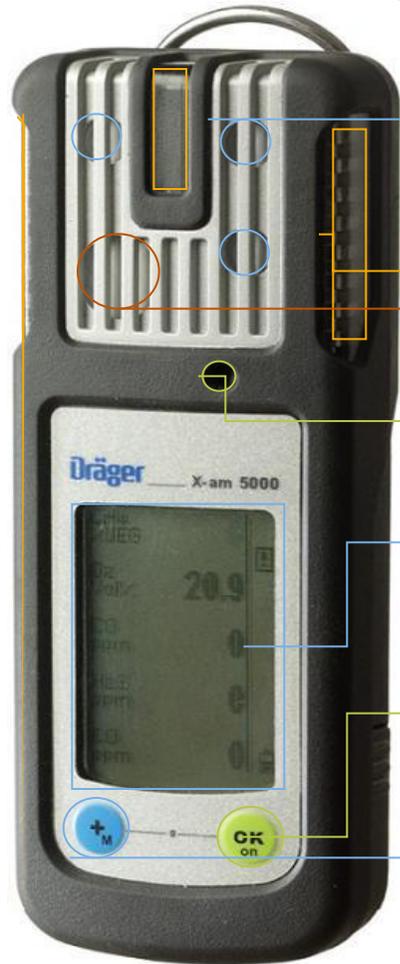

XXS sensor slot

Visual alarm

Catalytic sensor (X-am 5000) / IR sensor (X-am 5600)

Horn > 90 db

Segment display

**OK<sub>on</sub>** – Button  
Switch on  
Acknowledge

**+<sub>M</sub>** – Button  
Navigation

Operation X-am 5000/5600

### SWITCHING ON

Press and hold the “OK”-key for 3 seconds

- Display counts down 3-2-1
- blinking LEDs, the acoustic alarm sounds
- and the vibrating alarm pulsates

The self-test begins automatically and shows the following:

The installed software version

- The alarm levels
- The TWA and STEL alarm settings
- The next calibration date



## Dräger X-am 5000/5600 Switching off

### SWITCHING OFF

Press and hold the “+” and “OK” keys at the same time for more than 3 sec.  
The LEDs will flash and a beep will sound.  
The instrument is switched off



▶ Look at video

## Dräger X-am 5000/5600

### Display Illumination

#### DISPLAY ILLUMINATION

- Press any key and the display illumination is switched on for about 30 sec.
- In an alarm situation, the display illumination is automatically switched on



 Look at video

## Dräger X-am 5000/5600

### Menu Fresh Air Calibration



#### FRESH AIR CALIBRATION

This procedure is a fresh air calibration, which is placed in the quick menu with help of the CC-Vision Software.


- Press “+”-key three times
- The following con is shown 
- Press the “OK”-key and choose the fresh air calibration menu

Real values are shown

Press the “OK”- key

OK appears in the display

Fresh air calibration is finished

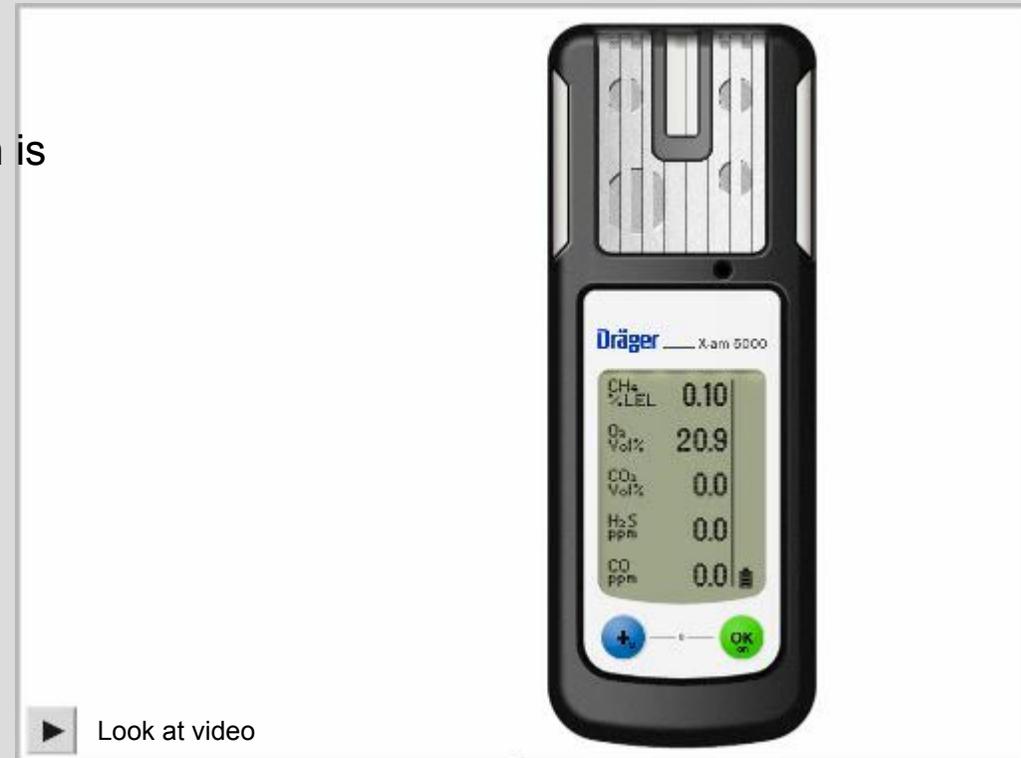

The fresh air calibration / zero point adjustment is not supported by the DrägerSensor Dual IR-CO2 and the DrägerSensor IR-CO2. A zero point calibration / adjustment of these sensors can be conducted using the Dräger CC-Vision PC software. To do so, a suitable zero gas that is free of carbon dioxide (e.g. N2) should be used.



# Dräger X-am 5000/5600



## Menu Maximum Value



### MENU MAXIMUM VALUE


Press and hold the “OK”-key for **3 seconds**

The Maximum Value and the minimum value for the O<sub>2</sub> sensor are shown. These values have been recorded since the last time the instrument was reset.

Press the “OK”-key again.

TWA and STEL values appear in the display or press the “+”-key once

Instrument returns to measurement mode

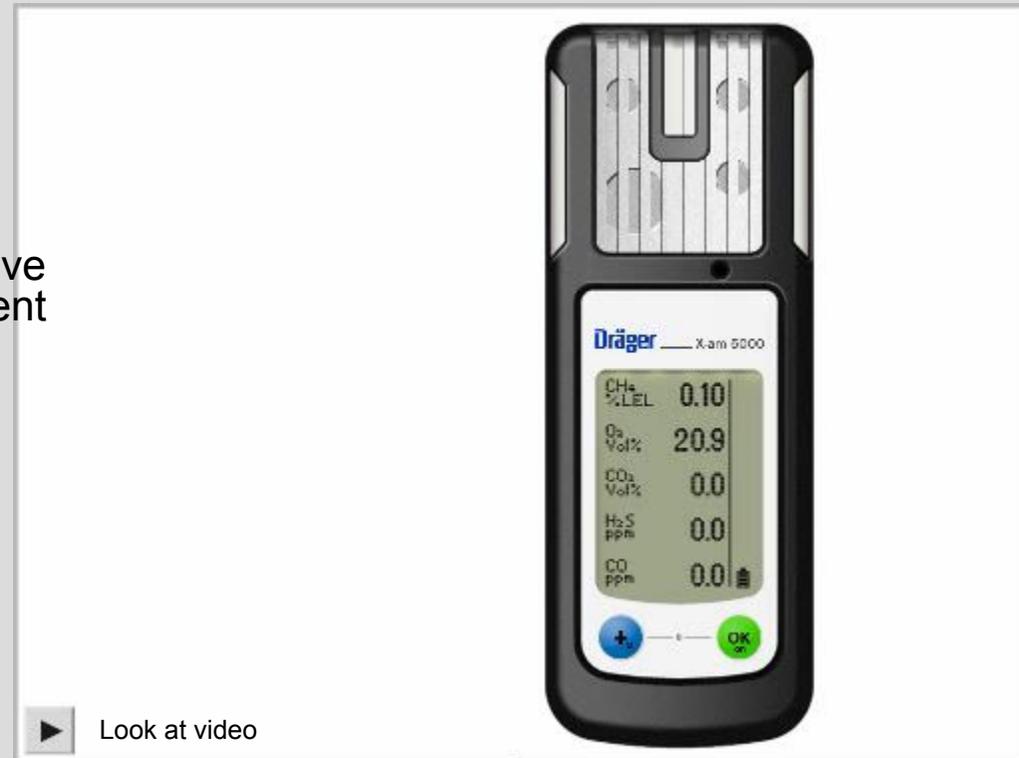

- The function Max Value displays the lowest oxygen reading and the highest readings for the other sensors from the time the readings were last reset.
- You can use the Max Value function in the quick menu (configurable with CC-Vision) to view and to reset the max values.



# Dräger X-am 5000/5600

## NOTE



TWA (Time Weighted Average) is the time-weighted average gas concentration (normally over an 8 hour period) that an unprotected worker can be exposed to over an 8 hour workday and 40 hour work week without adverse effects.



The STEL (Short Term Exposure Limit) is the maximum allowed gas concentration that an unprotected worker can be exposed within a 15 minutes period.



## Dräger X-am 5000/5600

### Menu Functions



#### TWA

When the TWA analysis is activated:

Press and hold the “OK”-key for **3 seconds**

Press the “OK”-key one time

icon appears in the display




The maximum workplace concentration is shown

Press the “OK”-key again and the STEL values are shown.

or press the “+,-”-key once

Instrument returns to measurement

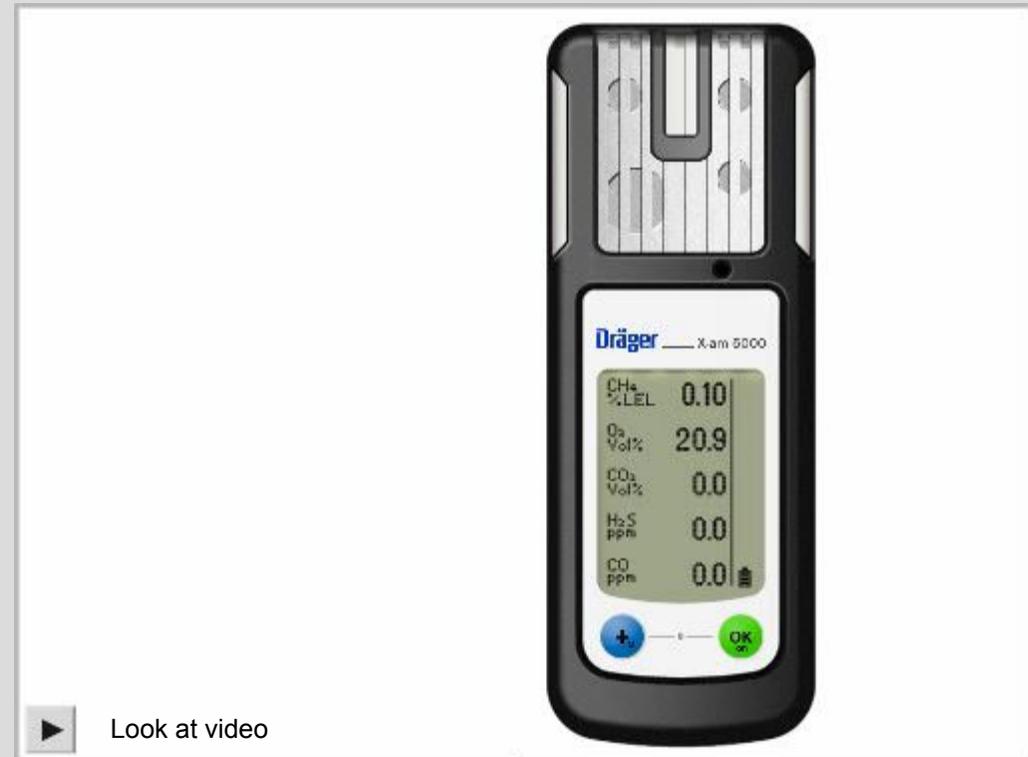

## Dräger X-am 5000/5600

### Menu Functions



#### STEL

When STEL analysis is activated:

Press and hold the “OK”-key for **3 seconds**


Press the “OK”-key two times

icon appears in the display 

The STEL values are shown

Press the “OK”-key or the “+”-key once

Instrument returns to measurement

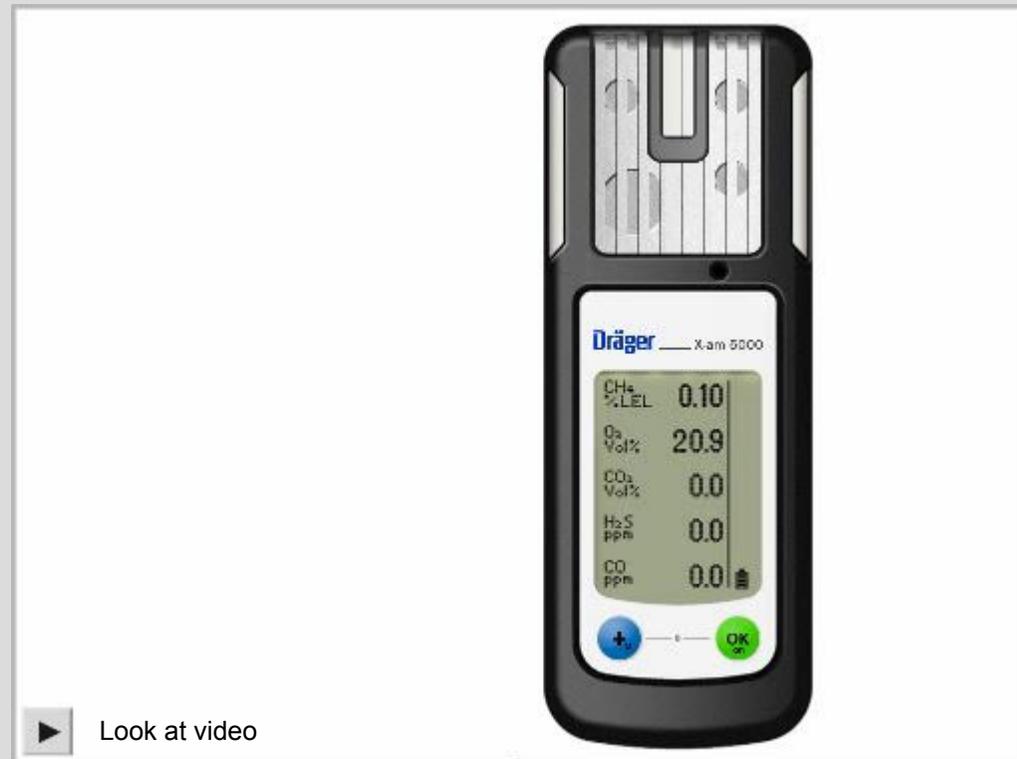

Look at video



# Dräger X-am 5000/5600

## A1 Gas Concentration Alarm

### A1 GAS CONCENTRATION ALARM

- Alarm level can be changed with the help of the CC-Vision software
- Audible-, visual- and vibrating alarms repeat periodically
- The display character “A1” will alternate with the concentration in the display
- An A1 alarm (except O2), the audible and vibrating alarms can be acknowledged by pushing the “OK”-key.



## Dräger X-am 5000/5600

### A2 Gas Concentration Alarm

#### A2 GAS CONCENTRATION ALARM

- Alarm level can be changed with the help of the CC-Vision software
- Double audible-, visual- and vibrating alarms repeat periodically
- The display character “A2” will alternate with the concentration in the display
- The audible, visual and vibrating alarms can NOT be acknowledged (silenced) in “A2” or in an O2 “A1” alarm



Follow the prescribed safety procedures.

## Dräger X-am 5000/5600

### STEL Alarm



#### STEL ALARM

- Alarm level can be changed with the help of the CC-Vision software
- Audible-, visual- and vibrating alarms repeat periodically
- The display character “A2” will alternate with the concentration in the display
- Icon  flashes
- The alarm can NOT be acknowledged



TWA and STEL values will be cancelled when the instrument is reset. Follow the prescribed safety procedures.



## Dräger X-am 5000/5600

### TWA Alarm



#### TWA ALARM

- Alarm level can be changed with the help of the CC-Vision software
- Audible-, visual- and vibrating alarms repeat periodically
- The display character “A2” will alternate with the concentration in the display
- Icon  flashes
- The alarm can NOT be acknowledged



TWA and STEL values will be cancelled when the instrument is reset. Follow the prescribed safety procedures.



# Dräger X-am 5000/5600


## A1 Low Battery Alarm



### A1 LOW BATTERY ALARM

- Audible-, visual- and vibrating alarms repeat periodically
- Icon  flashes
- The alarm can be acknowledged with “OK”-key

Click the picture to watch video

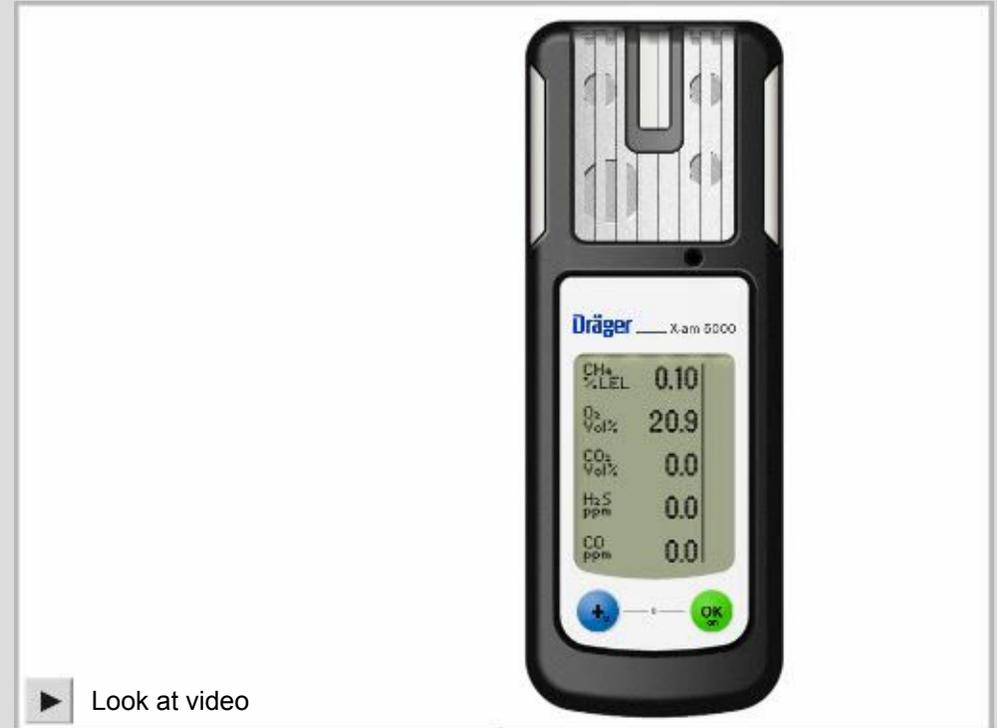

Look at video

This is activated when the battery has less than 10 minutes of operation – please change the batteries or charge the instrument.



# Dräger X-am 5000/5600

## A2 Low Battery Alarm



### A2 LOW BATTERY ALARM

- Audible-, visual- and vibrating alarms repeating periodically
- Icon  flashes
- The instrument will automatically shut down in about 10 seconds
- Instrument switches off
- The alarm can NOT be acknowledged



## Dräger X-am 5000/5600

### Error Alarm



#### ERROR ALARM

- Audible-, visual- and vibrating alarms repeat periodically
- The icon  appears in the display
- These alarms may be silenced with the “OK” - key, but the gas display will still indicate a fault



An error is an indication that something needs to be looked at in the instrument immediately. The instrument should be removed from service and the error corrected before further use



# Dräger X-am 5000/5600

## Over Range



### OVER RANGE

- Audible-, visual- and vibrating alarms repeat periodically
-  and A1 appear alternately
- The alarm can NOT be acknowledged



If the measuring range is exceeded, the following display is shown instead of measured value display. Follow the prescribed safety procedures.




# Dräger X-am 5000/5600

## Under Range



### UNDER RANGE

- Audible-, visual- and vibrating alarms repeat periodically
-  is shown
- The alarm can NOT be acknowledged

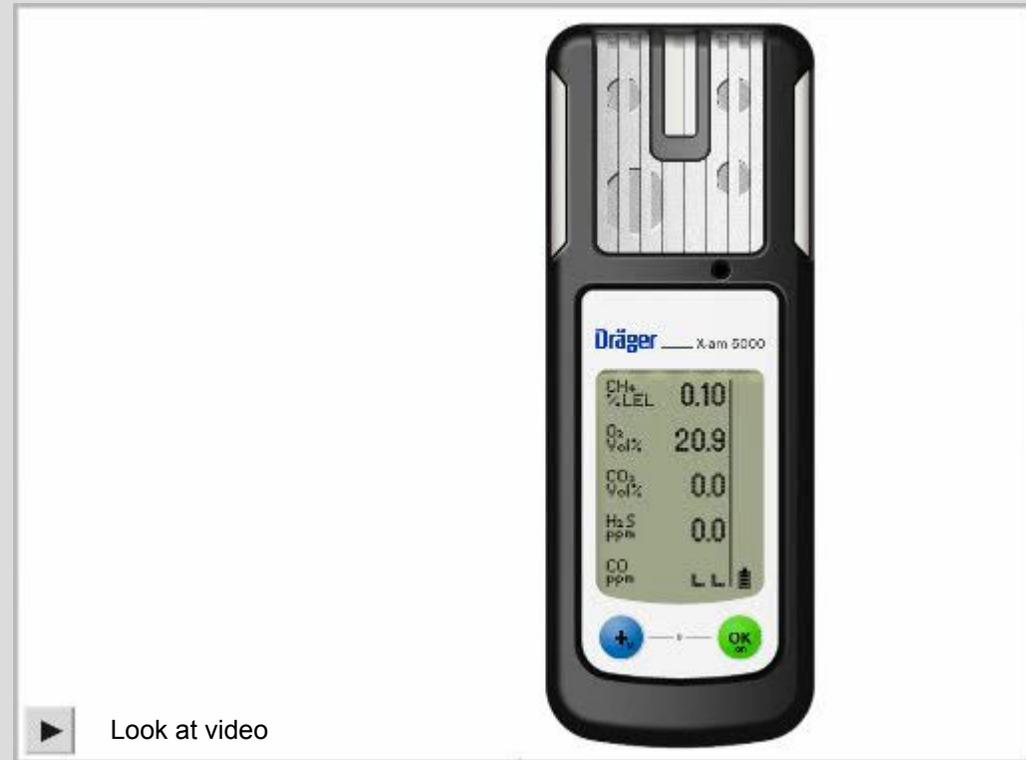


The measured concentration has drifted into the negative range. This can e.g. happen, when the fresh air calibration was done in an area where a concentration of gas was present. Please fresh air calibrate the instrument in a clean environmental.



### **X** ERROR DISPLAY

- Press the “OK”-key to acknowledge
- Press the “OK”-key again  
An Error code is shown  
(Use the instructions to determine what the error code means.)
- Press the “OK”-key again.  
More error code could be shown.
- Or press “+<sub>M</sub>”-key to return to measurement

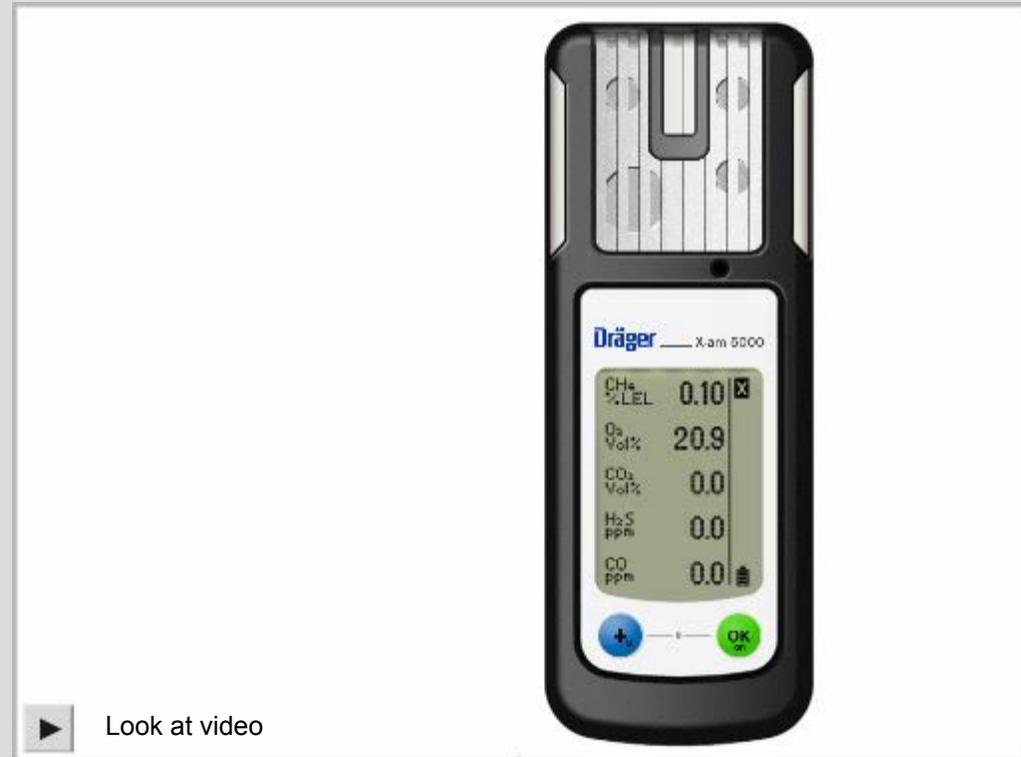


## NOTICE



### NOTICE

- Press the “OK”-key
- A Notice Code is shown  
(Use the instructions to determine what the notice code means.)
- Press the “OK”-key again.  
More notice codes could be shown
- Or press “+M”-key to return to measurement

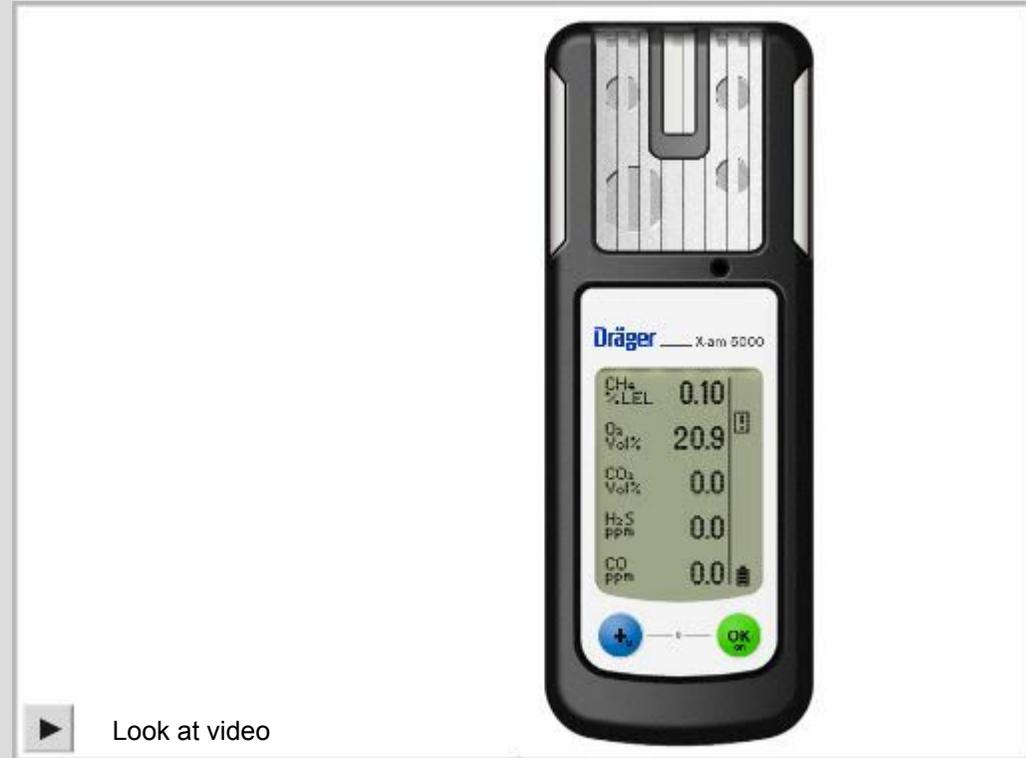

**Operation Pump for X-am 1/2/5000**

## Dräger X-am 5000/5600

### Confined Space Entry

#### STARTING THE PUMP FOR DRÄGER X-AM 1/2/5000

- Switch on the gas measuring device and insert it into the pump. It clicks into place.
- LEDs will light shortly green / red, a tone will sound
- The pump is automatically switched on and triggers the Flow-Test

- Flow LED flashes yellow, tone sounds
- Block the intake port for 2 seconds (by bending the hose)
- Flow LED flashes red, continuous tone will Sound
- Unblock the intake port
- Flow LED lights green
- The instrument is operational



the flow LED flashes red, accompanied by a continuous tone.

### OPERATION OF THE PUMP FOR DRÄGER X-AM 1/2/5000

- Performing the measurement:
  - Connect the Dräger sampling hoses or the Dräger probes to the hose connection of the pump
  - Perform the measurement
- Ending operation:
  - Press the release key
  - LEDs flash shortly green / red, short signal tone
  - The pump is switched off automatically



### Attention!

Before every measurement, flush the Dräger sampling hose or the probes with the air sample to be measured.



**Rule of thumb:** When using a new sampling hose, a typical flushing time of approx. 3 seconds is required for each meter. The sensor response time should be added.



Function test and Maintenance

# Dräger X-am 5000/5600

## Data Read Out

### DATA READ OUT

- In the display, “PC” appears when the instrument is connected via IR interface to a personal computer

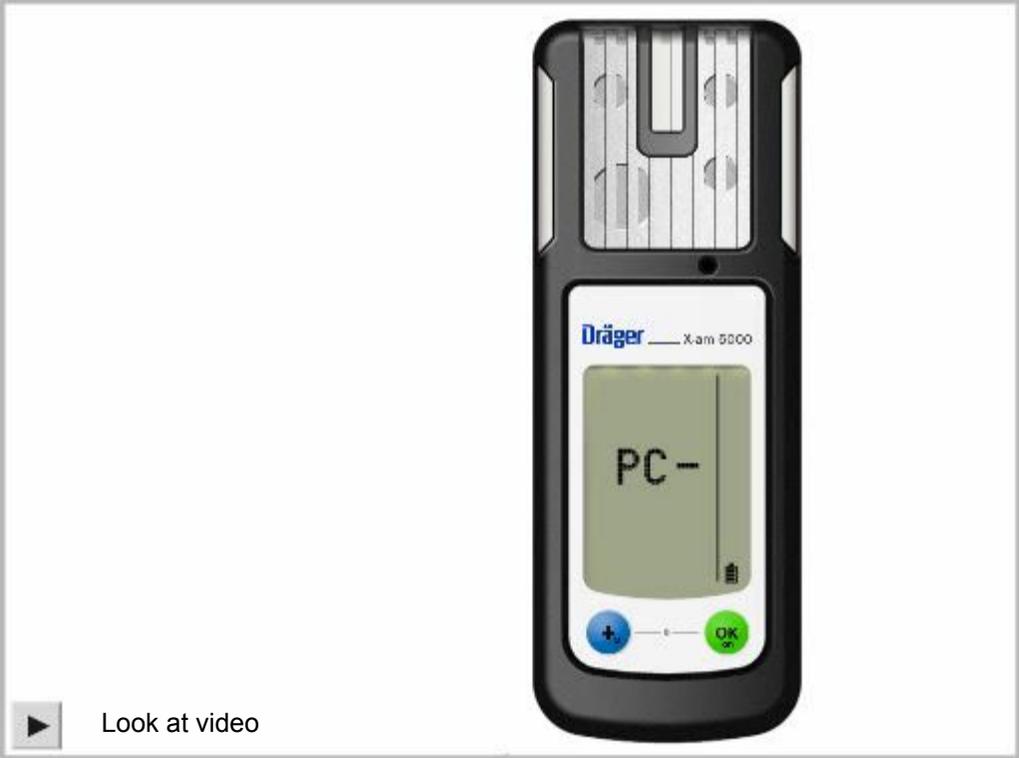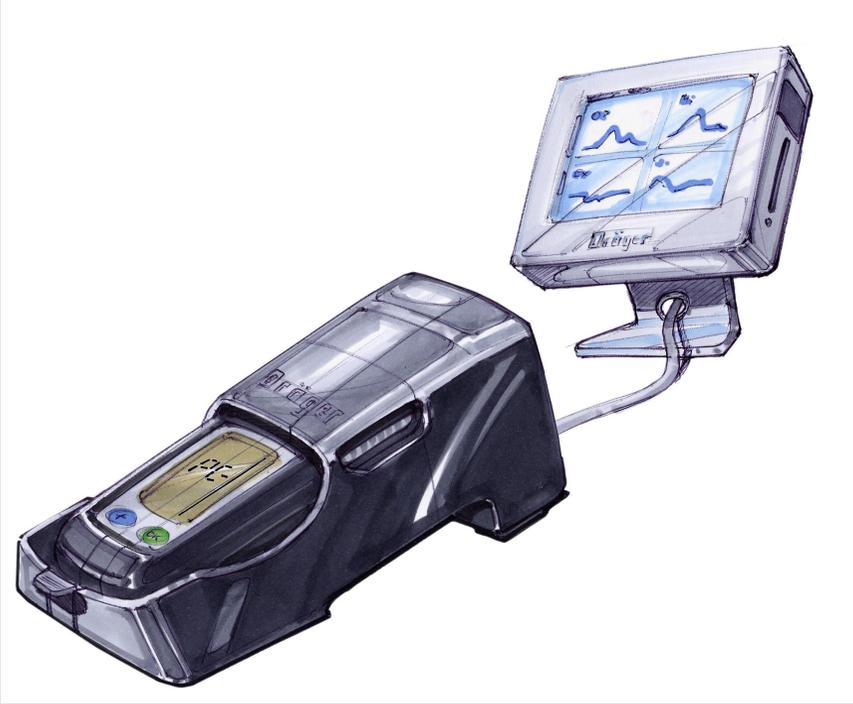

# Dräger X-am 5000/5600

## Function Test

- **A „Bump Test“ is a function test. Before using the instrument, it is important to check following:**
- Gas channels are not blocked (e.g. with dirty membranes )
- The sensors are calibrated correctly
- The correct alarms are shown
- The alarm levels have been adjusted correctly


## Dräger X-am 5000/5600

### Automatic Bump Test



#### AUTOMATIC BUMP TEST

- Slide the instrument into the bump test cradle
- The Bump Test Station automatically recognizes the instrument
- Gas is supplied to the sensors
- The values increase
- Audible and visible A1/A2 alarms are shown
- If the Bump test is correct, “ ” appears in the display
- The bump test is completed
- If the bump test is not correct,
- A channel error is shown for the specific sensor
- The instrument should be calibrated or contact your local service.

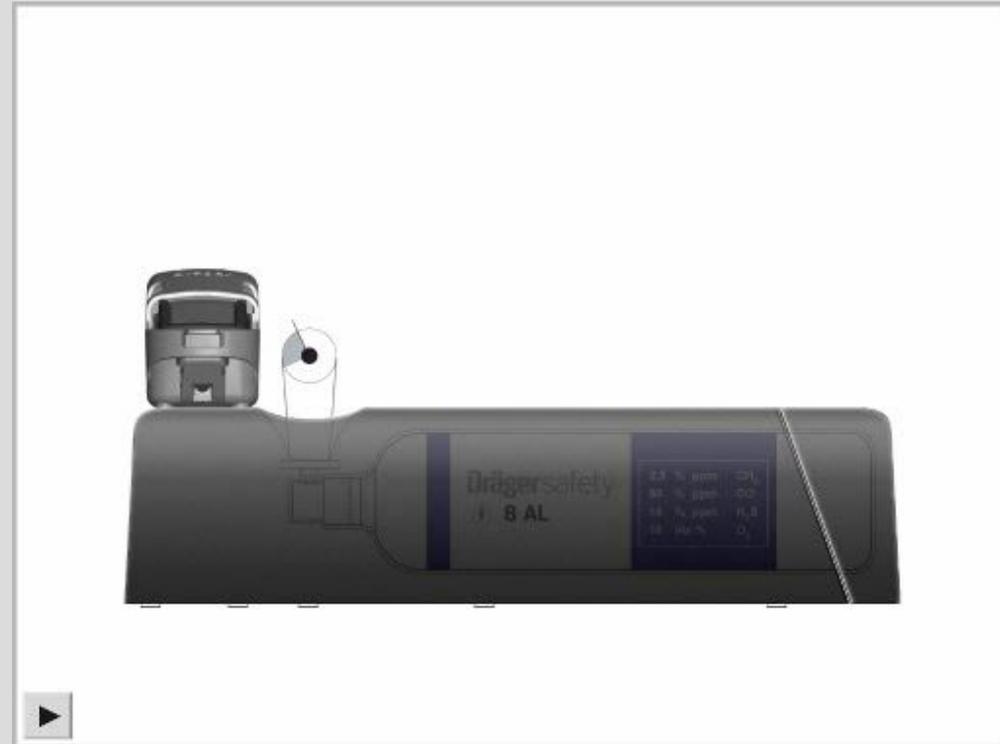



### MANUAL BUMP TEST

- Slide the instrument into the calibration cradle
- Press “+M”-key three times
- Manually supply the gas
- The values increase
- Audible and visual A1/A2 alarm are shown
- Press the “OK”-key
- The bump test is completed
- Or a channel error is shown for the specific sensor
- The instrument needs to be calibrated or contact your local service



# Dräger X-am 5000/5600

## Charging the battery pack

### CHARGING THE BATTERY PACK

- Slide the instrument into the charging module
- Connect the charging module with a single- or multi-charger
- The instrument is charging
- Red LED blinks -> instrument is charging
- Red LED lights stay on -> instrument is fully charged
- 4 hours are needed for a complete charge



Do not charge underground or in areas, where explosions can occur! There is a danger of explosion! The chargers are not designed in accordance with the regulations for fire and explosion protection..



# Dräger X-am 5000/5600

## Battery Case

### POWER SUPPLY

- Loosen the screw with the help of a Allen key
- Remove the battery case
- Insert the 2 alkaline- or NiMh batteries
- Pay attention to the polarity of the batteries
- Install the battery case and tighten the screw



Do not charge the battery in explosion hazard areas. Alkaline-Batteries are part of the Ex-approval. Only the following types should be used:

Energizer No. E91

Energizer No. EN91 (Industrial)


Varta Type 4106 (power one)

GP 180AAHC (rechargeable NiMH batteries)

The use of alkaline batteries other than those described above invalidates the intrinsic safety approval for the instrument and could result in unsafe operation.

## Overview of the icons

- **Special symbols provide a quick message about the instrument status**

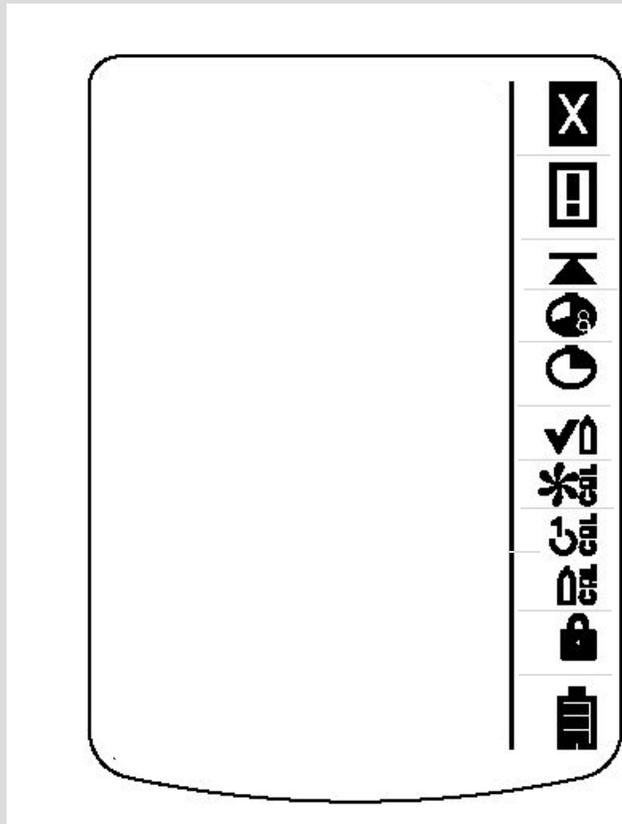

- Error Icon
- Notice Icon
- PEAK / Maximum Value Icon
- TWA Value Icon
- STEL Value Icon
- Bump Test Icon
- Fresh Air Calibration Icon
- 1-Button-Calibration Icon
- Span Calibration Icon
- Password-Protected Menu
- Battery Icon

THANK YOU FOR YOUR ATTENTION!