

Critical Path Research: Getting New Technology from Bench to Bedside A Device Perspective

**FDA Science Board
November 5, 2004**

**Dan Schultz
Director, CDRH**





Role of FDA

Establish reasonable
assurance of the safety and
effectiveness of medical
devices marketed in the U.S.

What is a “Device”?



A Computer You Can Swallow

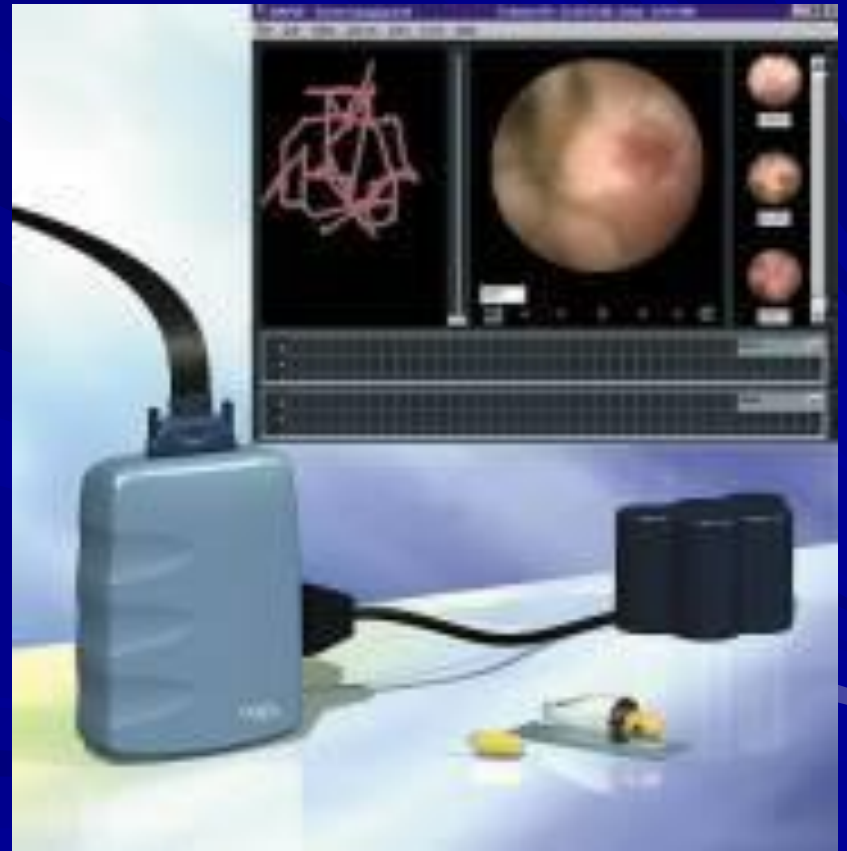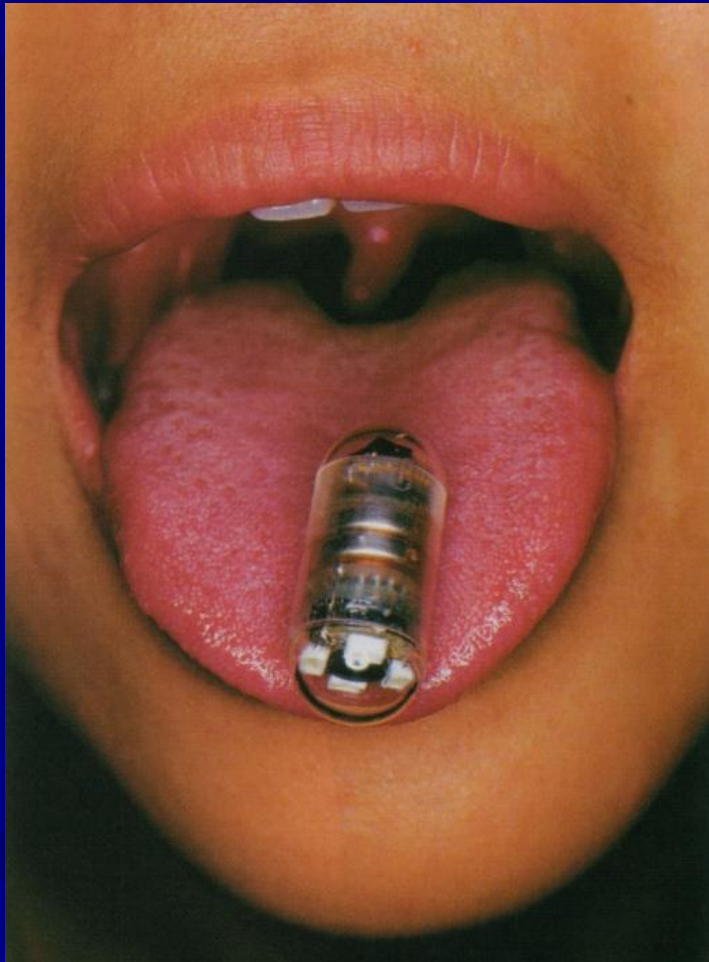

A Computer That Helps You Hear



Devices that Measure Glucose Levels and Deliver Insulin to “Communicate”




Miniaturized Electrical Stimulators

Pacemakers



Drug-Eluting Stents

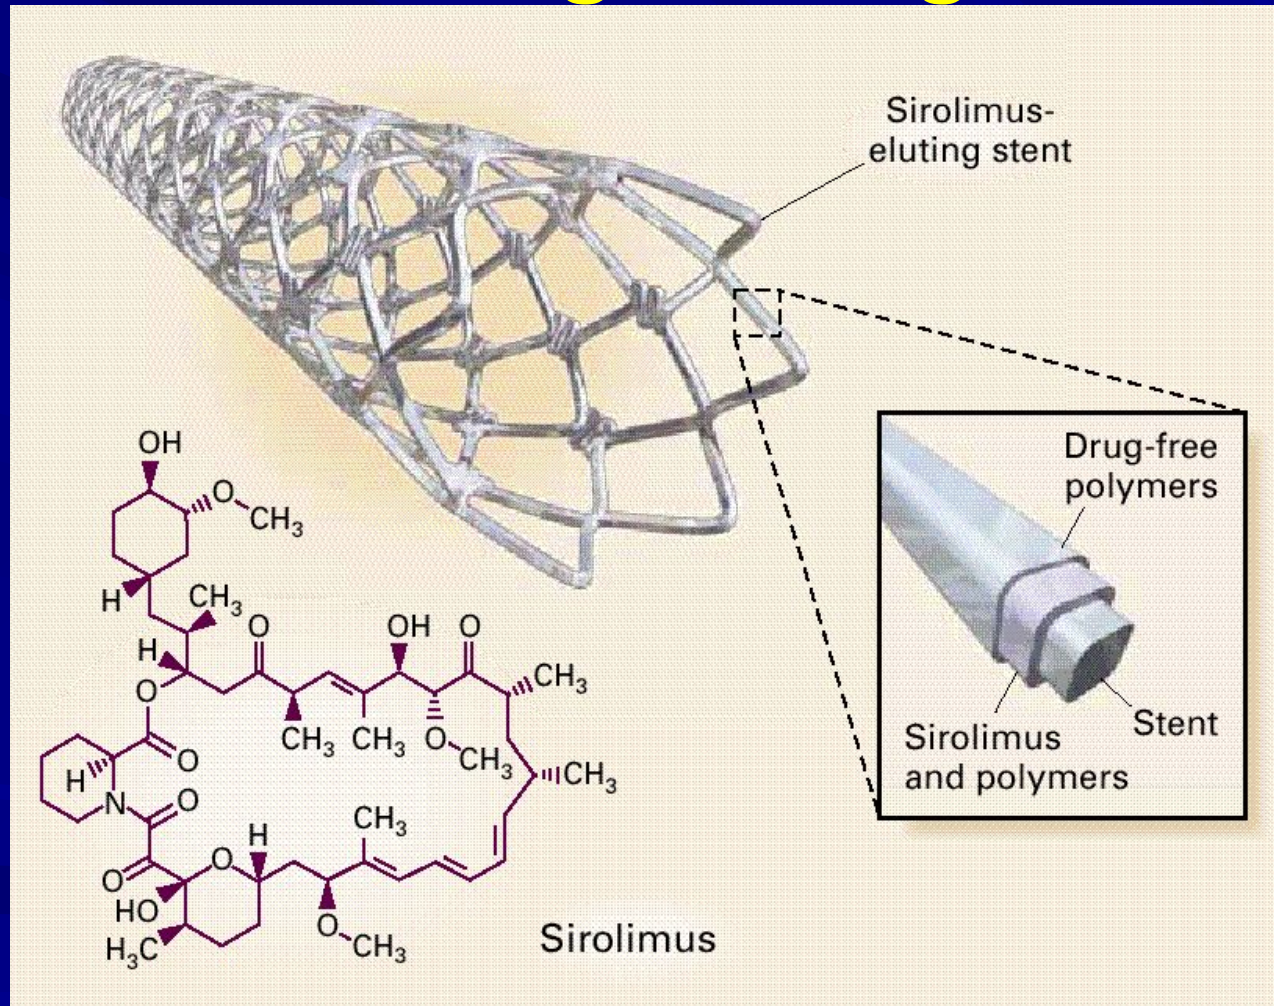


Components

- Stent Platform & Delivery System
- Carrier(s)
- Drug


New Technology

Important Trends

- Miniaturization
- Intelligent Devices
- Designed for Consumer Use
- Minimally invasive
- Biotechnology Revolution
 - Genomics, Proteomics
 - Biological Medical Devices
- New Materials
- Combination Products
- Disruptive Technologies
 - That change how we do business
 - That change how medical devices deliver value

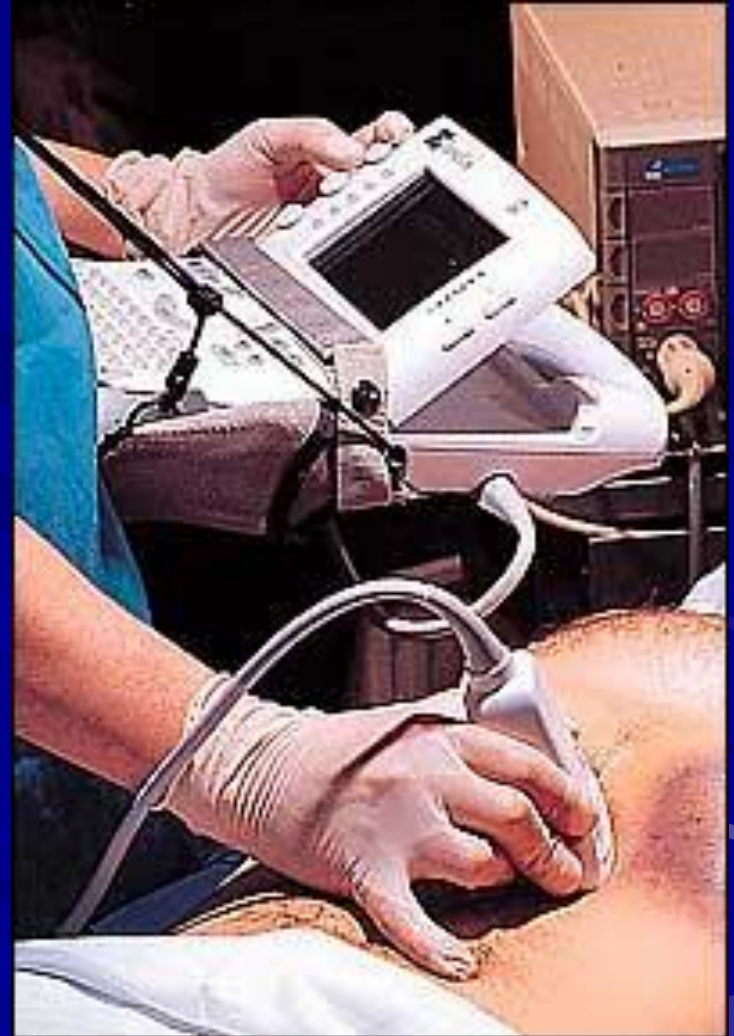

CDRH Vision – Total Product Life Cycle

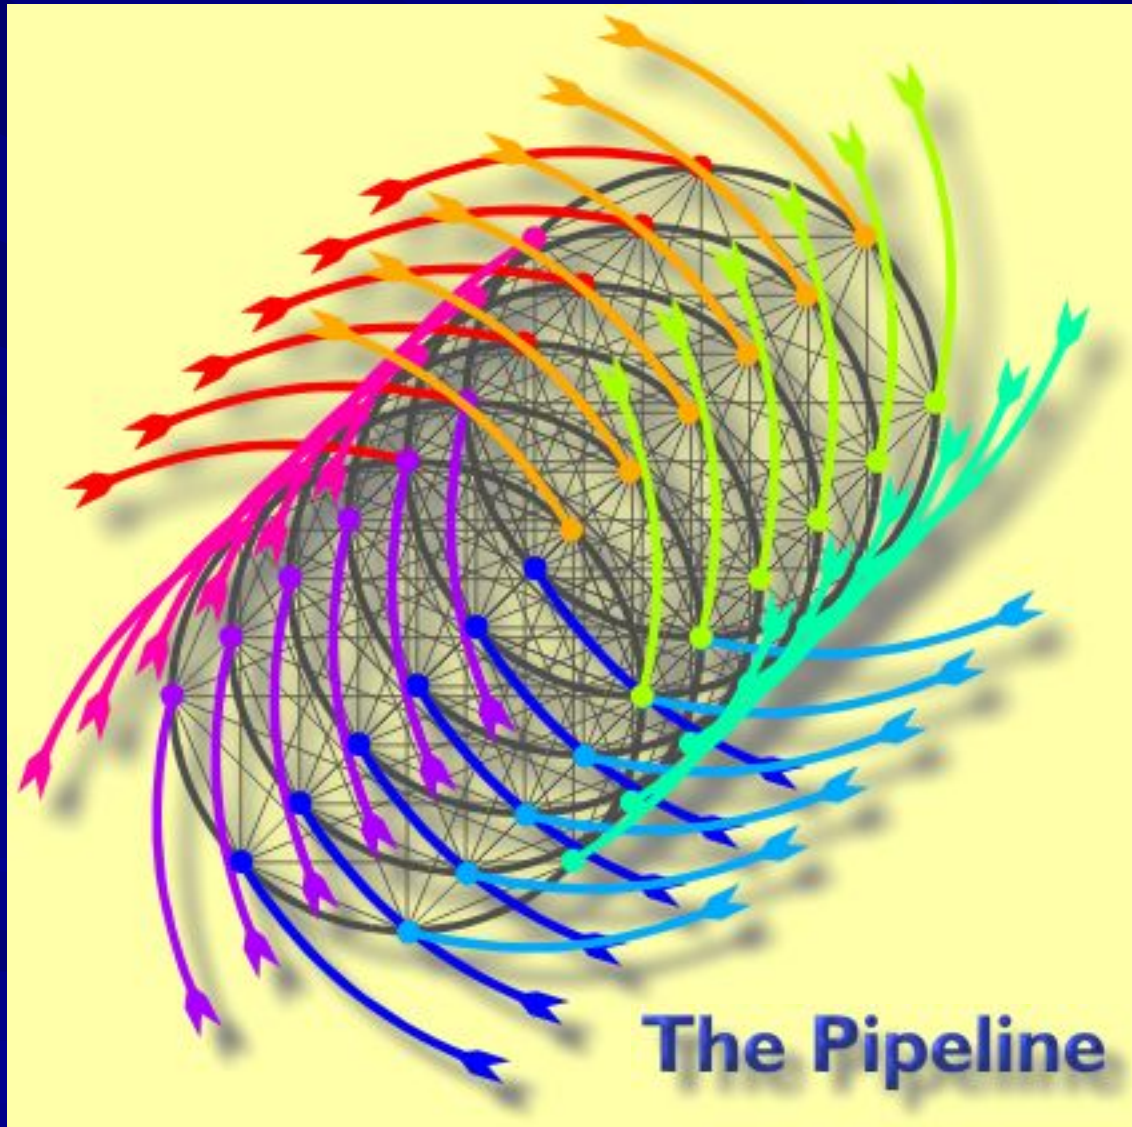

Devices are Different

- **Drugs**

- Pure molecules
- Toxicology
- Short half-life
- Long market life
- Drug interactions
- Wrong Drug / Dose
- Clinically studied
- Good Manufacturing Practices (cGMP)

- **Devices**


- Complex components
- Biocompatibility
- Durable Equipment
- Rapid product cycles
- Malfunction
- User Error
- Bench studied
- Quality Systems (ISO 9000)

Critical Path is Different for Devices


- **Device Regulation**
 - Least Burdensome Provision of FDAMA
 - Quality Systems and Design Controls
- **Device Innovation Process**
 - Biocompatibility
 - Iterative Process
 - User learning curve
 - Performance and durability
- **Device Industry is Represented by Small Manufacturers**

Medical Device Industry Growth

Number of Manufacturers by Year

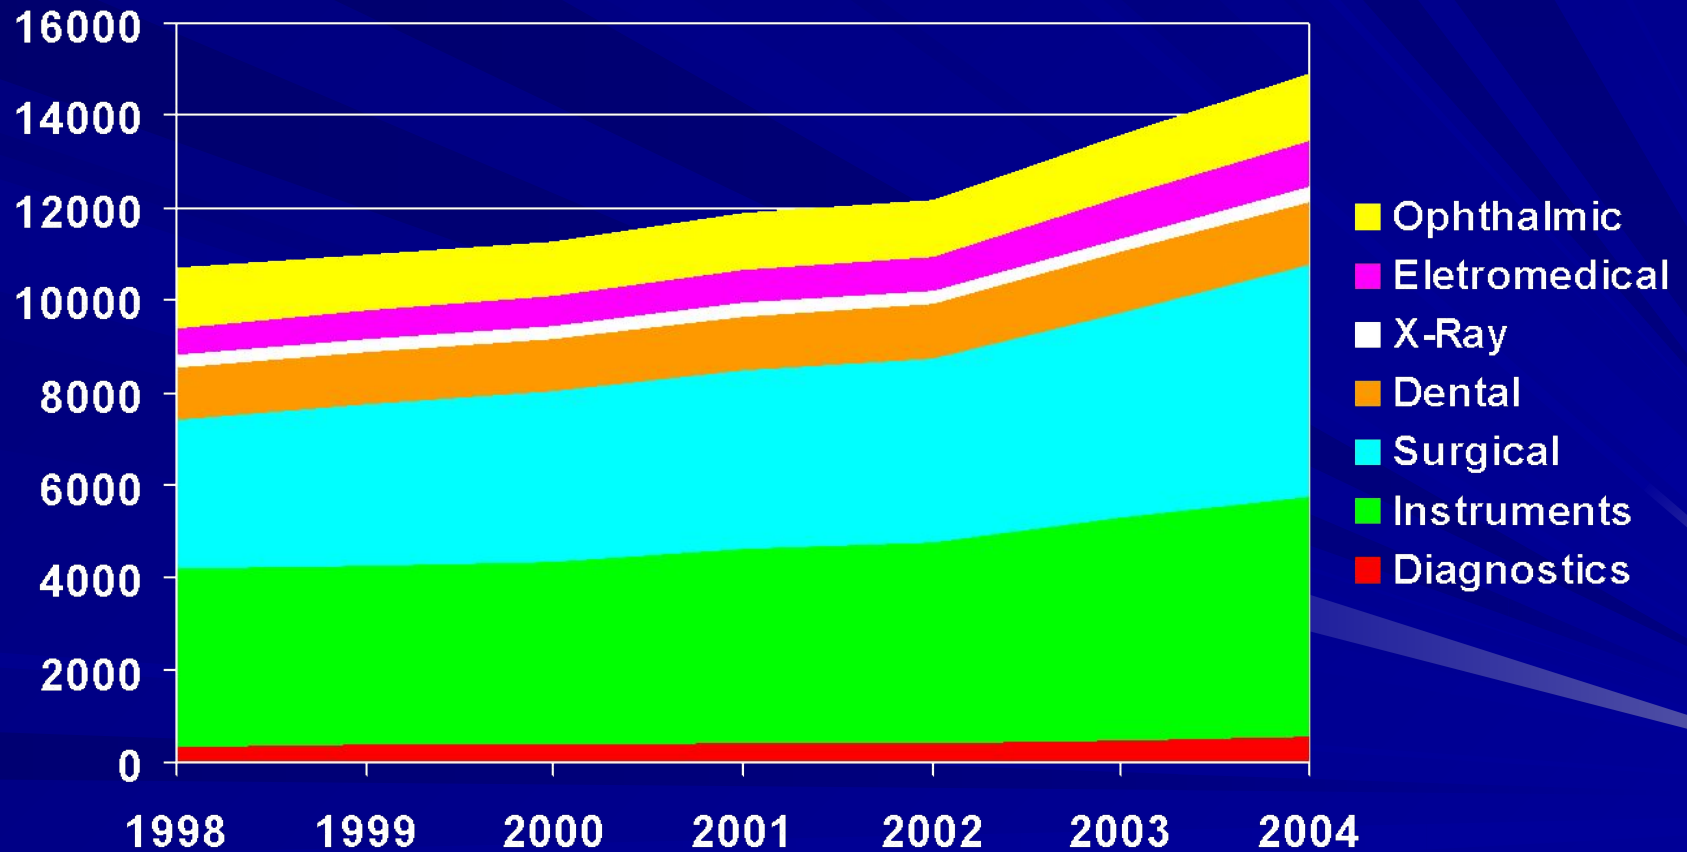

Sales Volume Growth (Billions of Dollars)

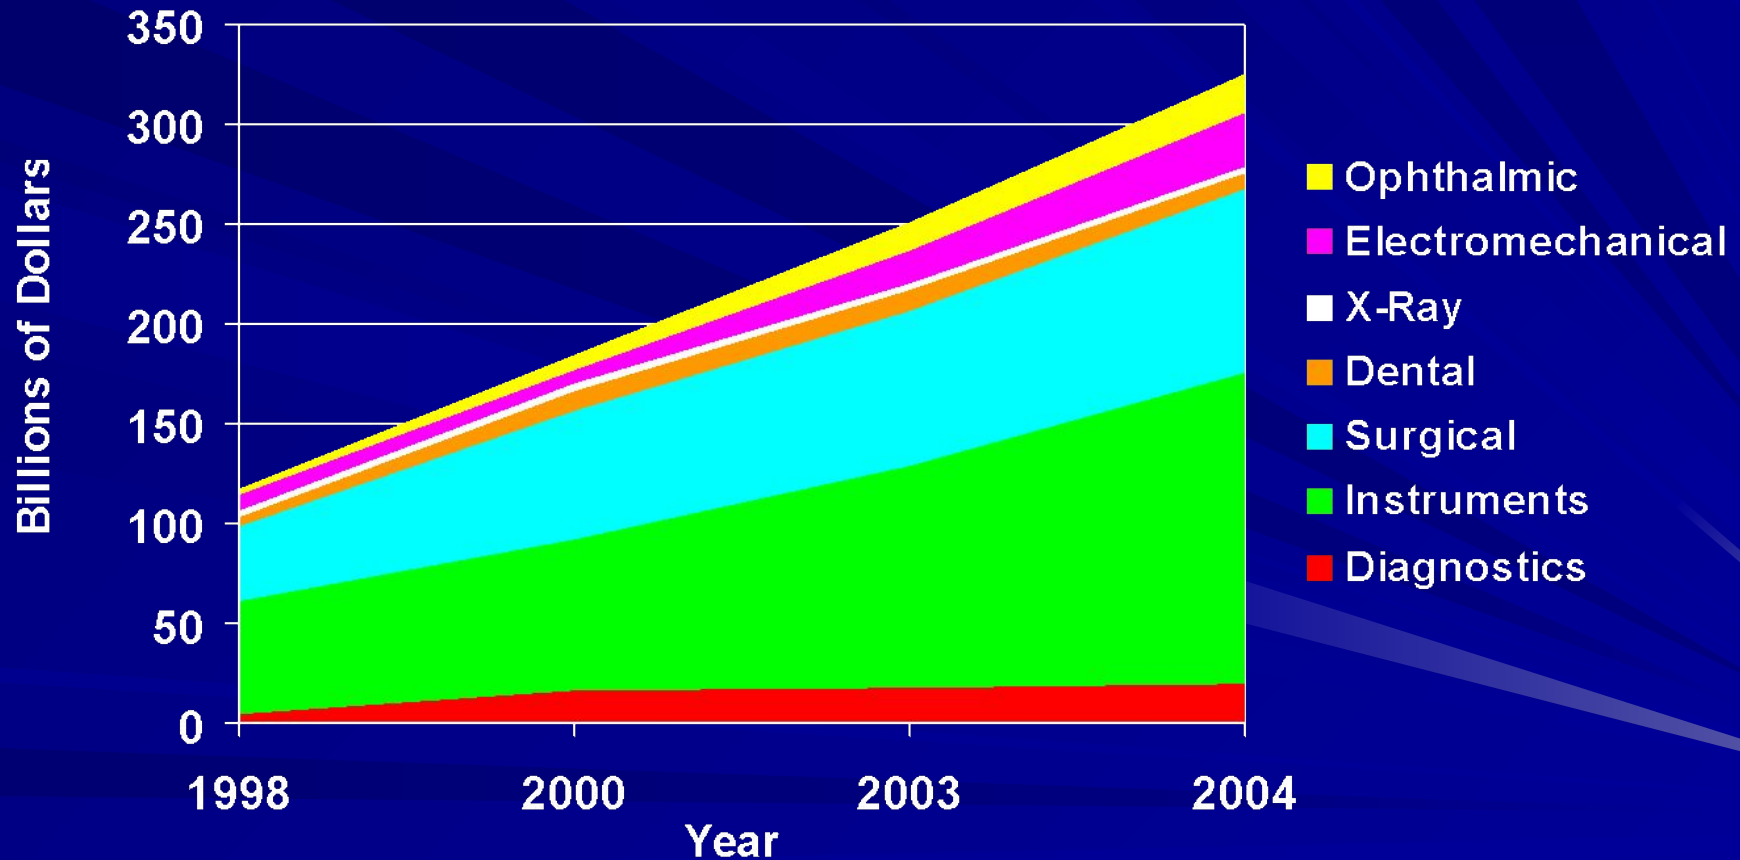

Note: No Economic Adjustment to Dollar Value


Device Industry Continues to Grow in FY 04

- **Dun and Bradstreet FY 04 data shows the device industry grew from 13,579 to 14,937 firms with about \$320 billion in sales.**
- **Innovation is alive and well!**
- **20% annual turnover in individual device firms.**
- **FDA-industry interaction is more important than ever. FDA needs to keep guidances and reviewers up to date.**

Innovative Science-based Strategies at Work


- **Leveraging**
 - Breast Cancer (DMIST): Screening and Digital Mammography
 - Medical Device Fellowship Program
- **Objective Performance Criteria**
 - Heart valves
 - Hip implants
- **Novel Trial Designs**
 - Bayesian Statistics
 - ROC Curves
- **Guidance Development**

Comparison of 510(k) Average Review Times for Devices With and Without Guidance*

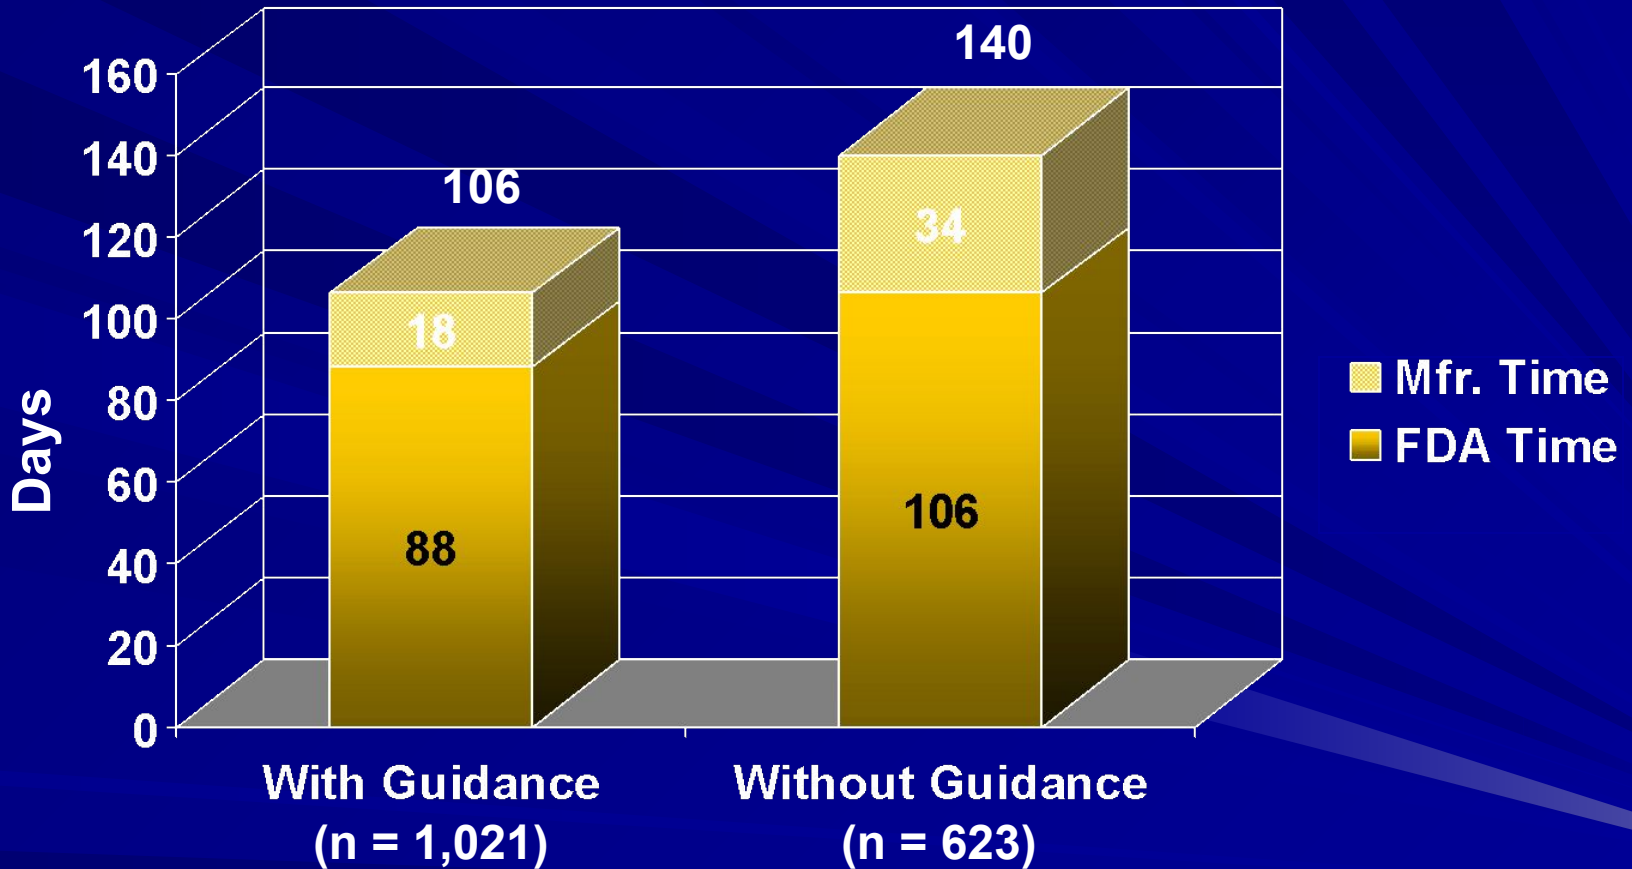


*Based on all 510(k)s (1,644) with SE decisions during FY 2002 that were for Class II devices eligible for third party review, excluding special and 3rd party 510(k)s

Original PMA Milestones: 2-cycle Scenario

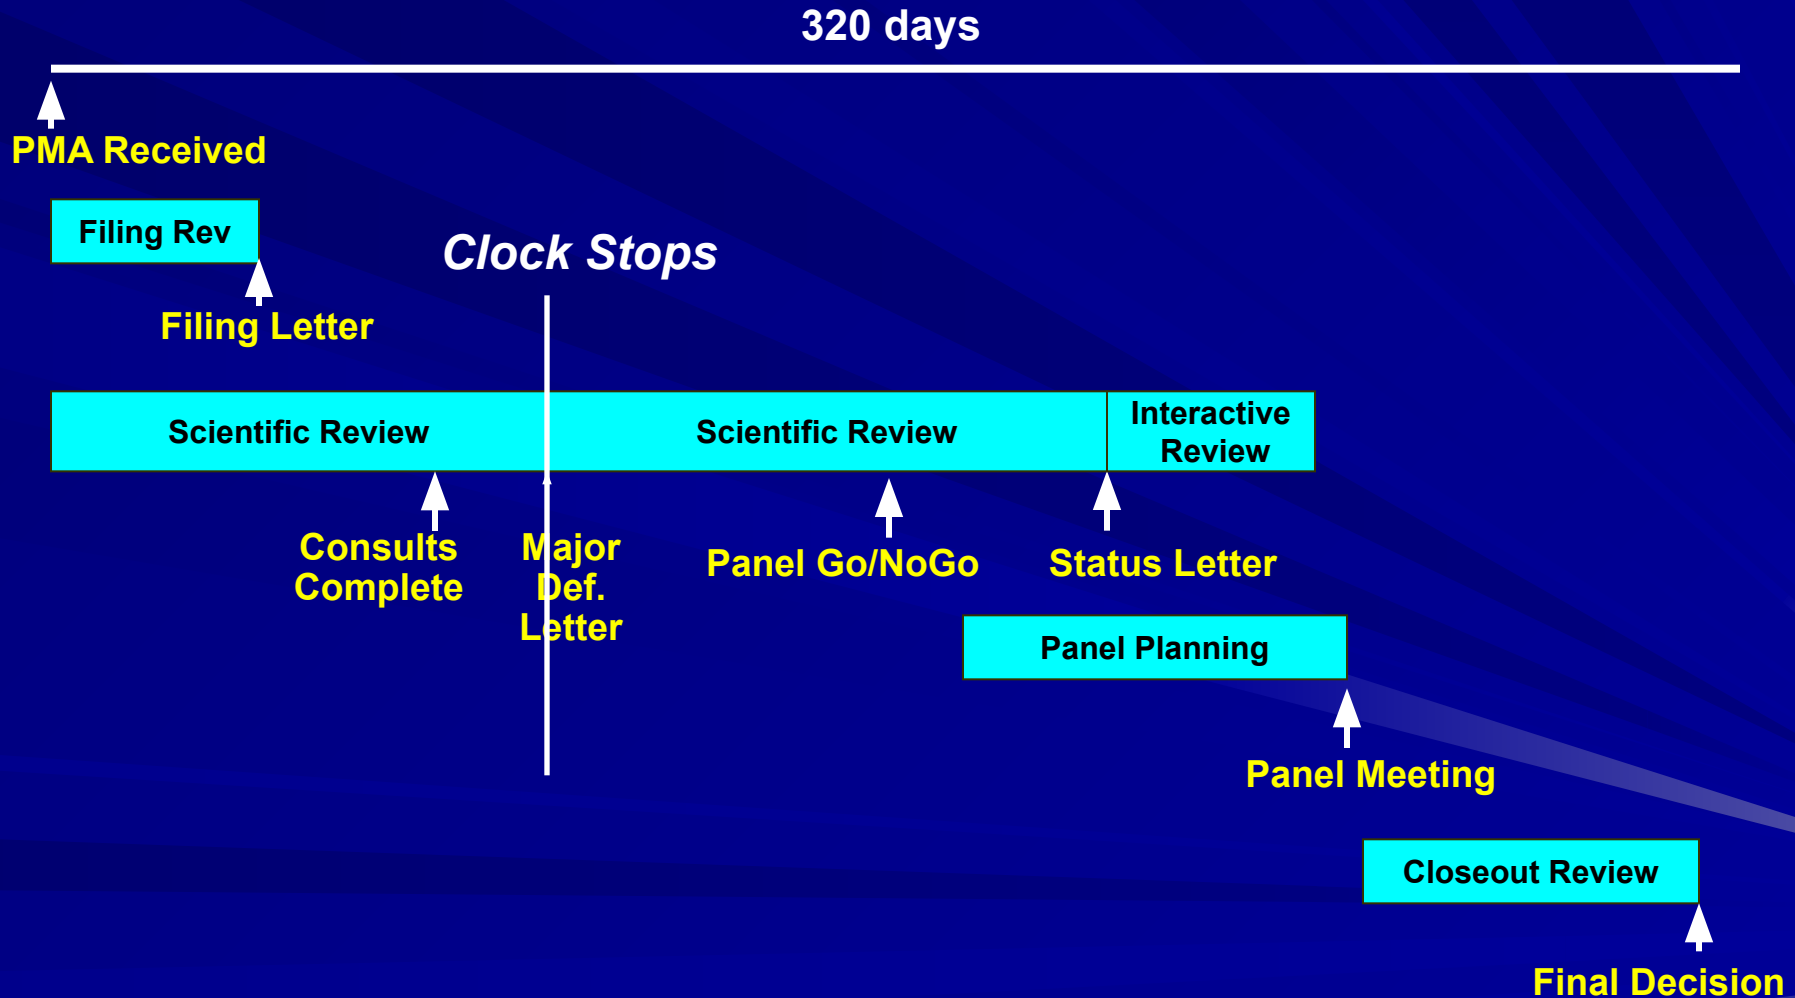

Original PMA Milestones: 1-cycle Scenario

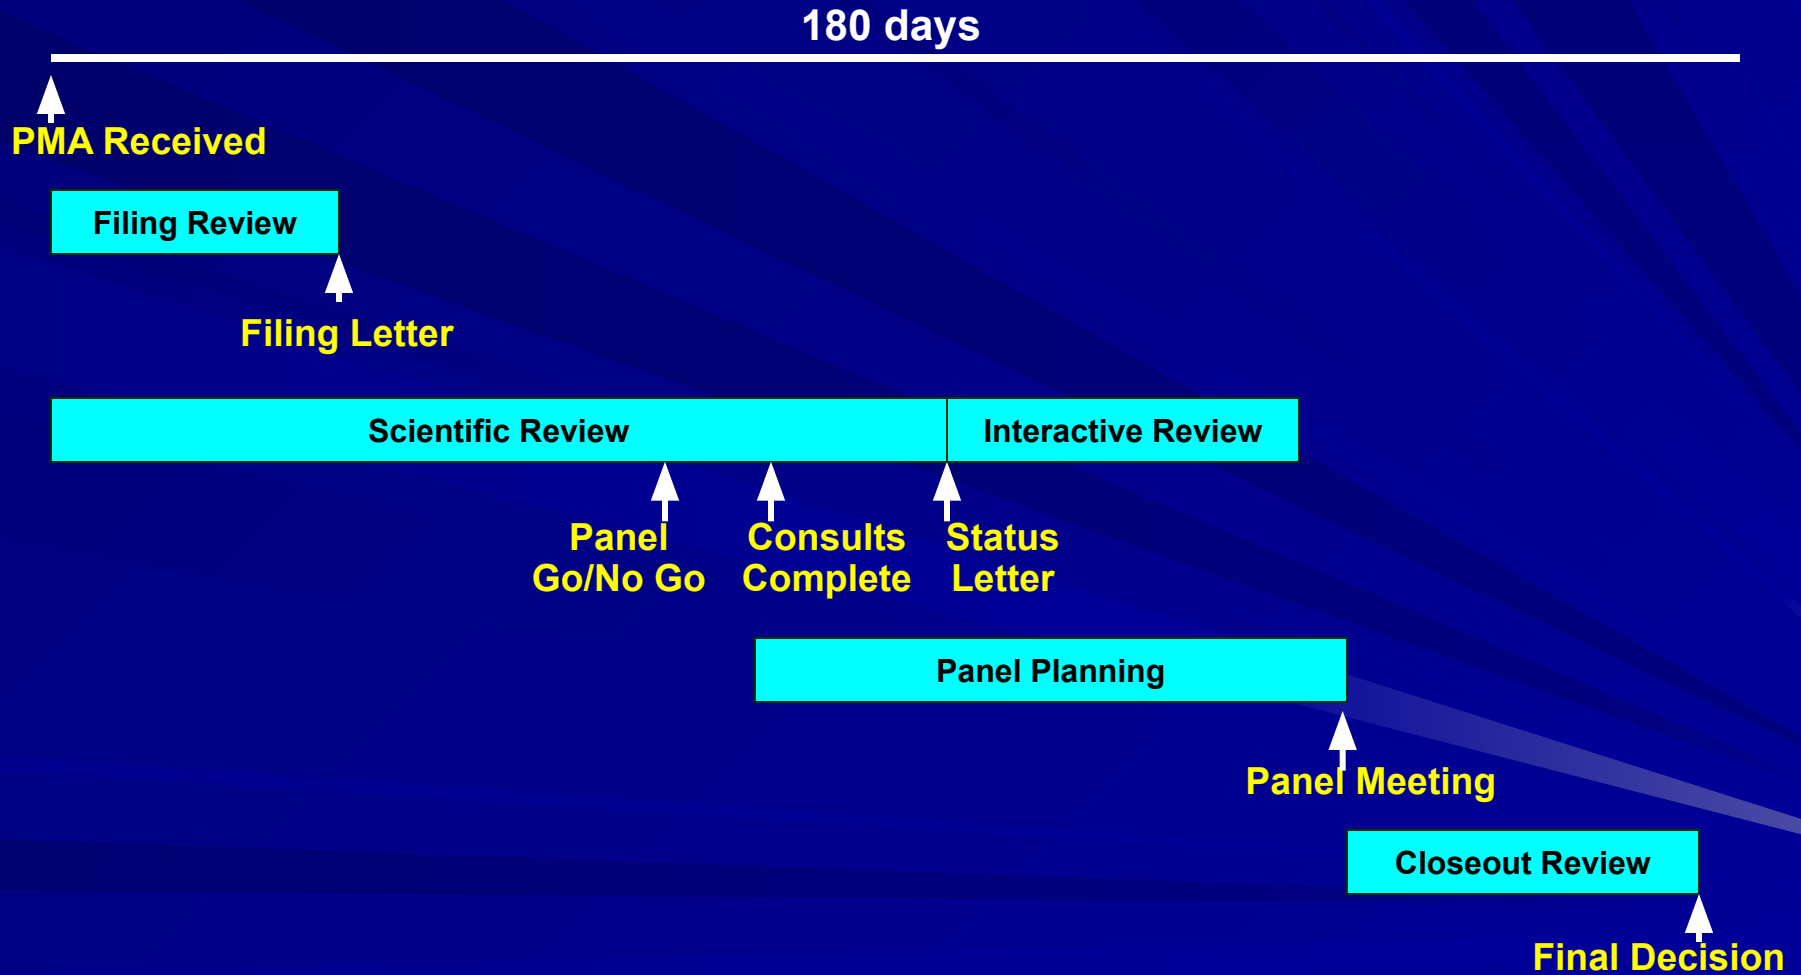

The rest of the story...



DICKINSON'S
FDA Webview

**Boston Scientific Stent
Recall Grows to 96K Units**



WSJ.com
THE WALL STREET JOURNAL.
ONLINE

**FDA Is Reviewing
Reports of Trouble With
Taxus Stent**

**Boston Scientific's Older Stents
Draw
Scrutiny of FDA**



The Boston Globe

**Boston Scientific Expands Recall
of Troubled Stent**

FDA won't expand recall of stents

**Drug-coated stents may face
additional FDA scrutiny**



The Miami Herald

**FDA Temperature
up over Cordis**





U.S. Food and Drug Administration



**FDA Advises Physicians of Adverse Events
Associated with Cordis Cypher Coronary Stents**


Goal: Prioritize Actions on GMP Risks Correlating to Patient Risks

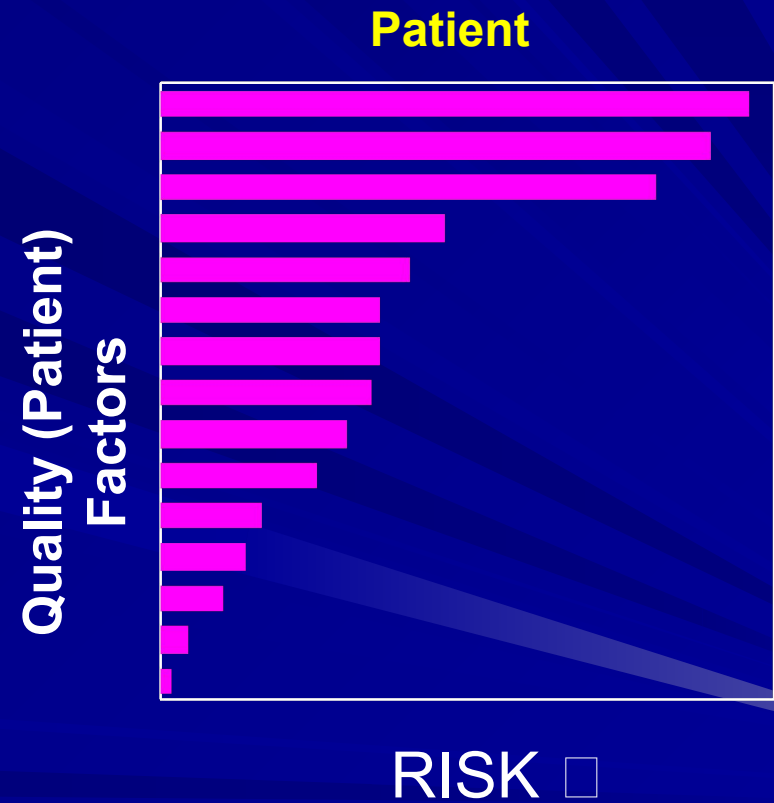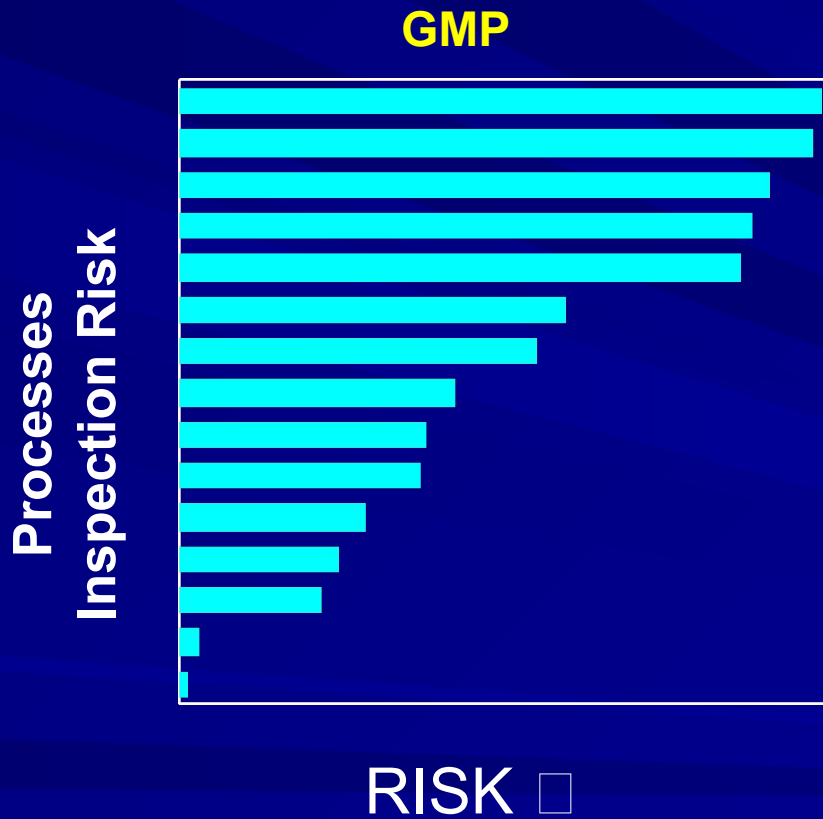

Postmarket Questions of Interest

- Long Term Safety
- Performance in Community Practice
- Change in User Setting
- Rare/Unexpected Events
- Rates of Anticipated Adverse Events
- Human Factors Issues – Use Error
- Off-Label Use

Achieving Pre/Postmarket Balance

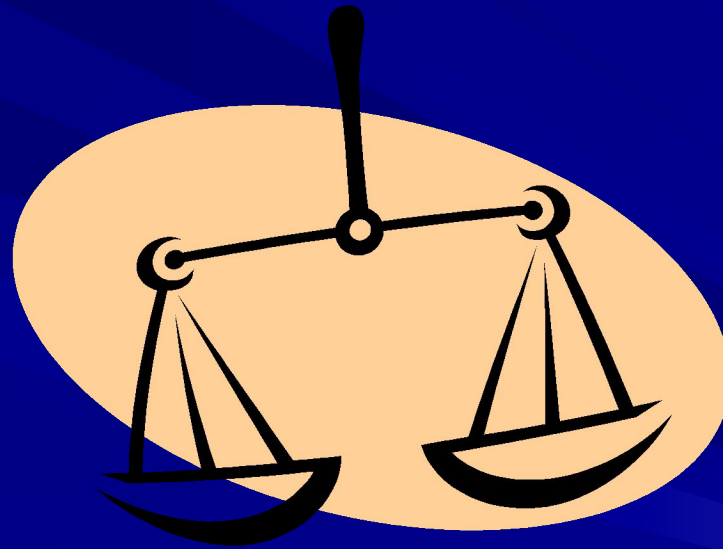

Why Balance Works

- **Speeds Product to Market by Moving Some Premarket Requirements to Postmarket**
- **Offers Added Assurance to FDA and Advisory Panel**
- **Free Up ODE Staff for Premarket Review**
- **Generates Data for Next Generation**
- **Generates Data for Enhanced Labeling**

Postmarket Studies - Present

- **III-Conceived**
- **Not Initiated**
- **Not Completed**
- **Not Tracked**
- **Not Enforced**

Postmarket Studies - Future

- **Better Designs**
- **Standardized Reporting System**
- **Better Tracking**
- **Make Status of Studies Public**

Life Sciences Laboratory

Awards

2004, GSA Construction Excellence, Projects Over \$25 Million

2004, Washington Building Council, Craftsmanship Award (Mechanical / HVAC-Sheet Metal, Mechanical / Plumbing, Mechanical / HVAC-Piping)



Critical Path Projects Being Developed

- **Establishing a pedigreed and credentialed blood panel that could be used for assessing the sensitivity/specificity of new hepatitis assays**
- **Developing computer models of human physiology that allow testing and soft failure of peripheral vascular stents before animal and human studies are ever considered**
- **Developing a clear regulatory path with consensus from the Obstetrics community for intrapartum fetal diagnostic devices**

Critical Path Projects Being Developed

- **Establishing agreed pathways for the statistical validation of surrogate markers**
- **Working with Medical Specialty Organizations to develop practice guidelines for appropriate monitoring of permanently implanted devices**
- **Obtaining consensus on the extent of neurotoxicity testing for neural tissue contacting materials**

Summary

- **Steady progress towards meeting review performance goals and TPLC strategic goals**
- **Success is achievable but highly resource-intensive**
- **CDRH continues to seek innovative methods and partnerships for evaluating new technology based on sound science in a least burdensome manner**
- **Critical path will further our existing efforts to achieve the right regulatory balance and ensure the safety and effectiveness of medical devices**

CDRH Vision – Total Product Life Cycle

